

cooltone™
by  coolsculpting®

Explore your options in body contouring



Indications



The CoolTone™ device is indicated for improvement of abdominal tone, strengthening of the abdominal muscles, and development for firmer abdomen. CoolTone™ is also indicated for strengthening, toning and firming of buttocks and thighs.

Important Safety Information

CoolTone™ should not be used in the head or heart area. CoolTone™ treatment is contraindicated in placing the active applicator over metal or electronic implants/devices in the treatment area like cardiac pacemakers, cochlear implants, intrathecal pumps, implanted defibrillators, implanted neurostimulators, drug pumps, and hearing aids. CoolTone™ is also contraindicated in placing the active applicator over menstruating uterus, over areas of the skin that lack normal sensation, and for patients with fever, malignant tumor, hemorrhagic conditions, epilepsy, recent surgical procedure application in the area of growth plate, pulmonary insufficiency, pregnancy, sensitivity or allergy to latex.

Please see additional Important Safety Information throughout.

Explore your options

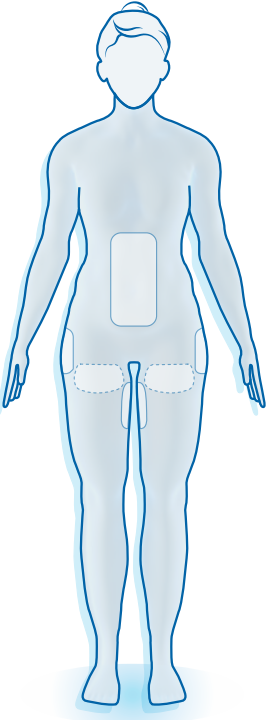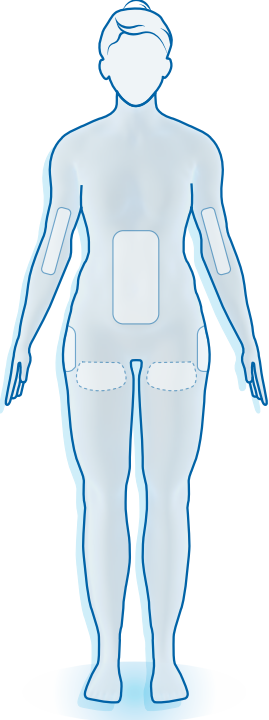	cooltone™	Competitor
Modality	Electromagnetic muscle stimulation (MMS) for muscle strengthening, toning, and firming	HIFEM® is a trademarked acronym for high-frequency electromagnetic muscle stimulation, which is the same as electromagnetic muscle stimulation ¹
Treatment Areas	<div><ul style="list-style-type: none">• Abdomen• Buttocks• Thigh</div>	<div><ul style="list-style-type: none">• Arm• Abdomen• Buttocks• Thigh</div>
	3 FDA-cleared treatment areas ¹	4 FDA-cleared treatment areas ¹

Important Safety Information (continued)




CoolTone™ should be used with caution in patients with Grave’s disease, active bleeding disorders or seizure disorders.

Women who are close to menstruation may find that it comes sooner or cramping is increased or intensified with CoolTone™ treatments, therefore it is recommended to not undergo treatment during this time of the month.

Please see additional Important Safety Information throughout.

A closer look at magnetic muscle stimulation systems

The clinical significance of these data has not been established.

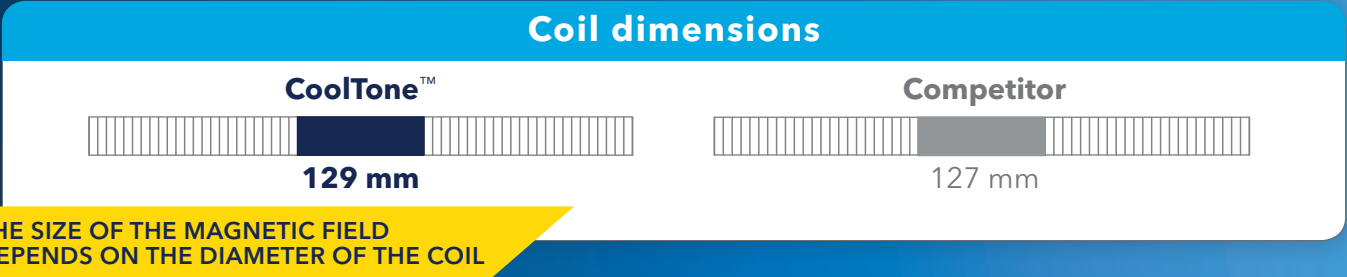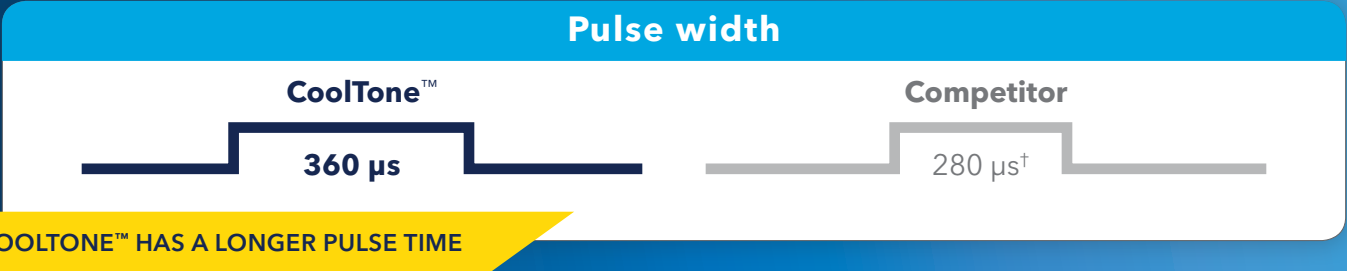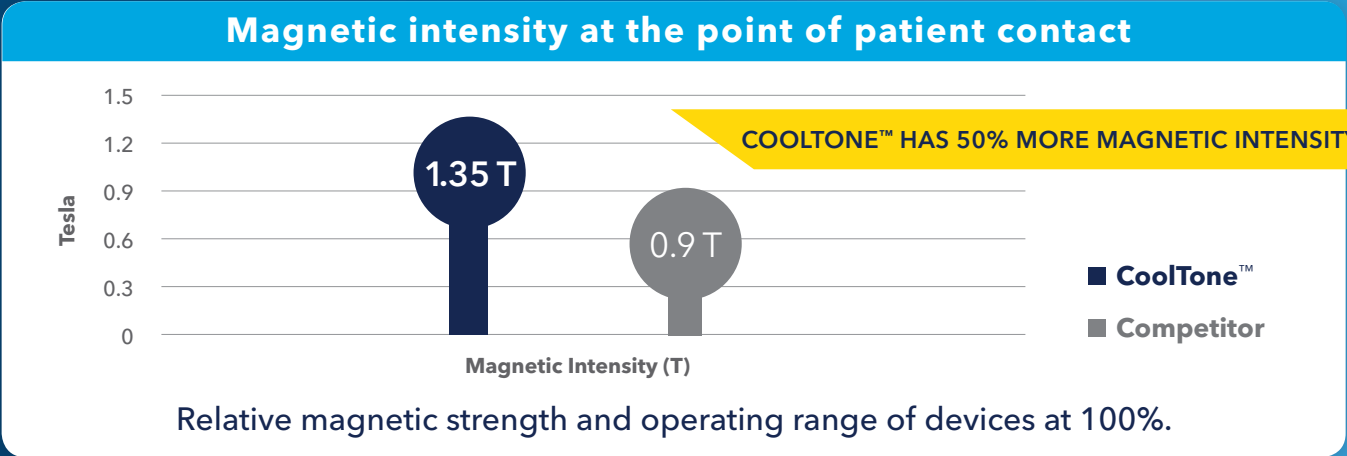

*Based on performance testing measuring magnetic field expressed in tesla (T) over the applicator surface.
†Magnetic field pulse width (+/- 20%).

Important Safety Information (continued)

Ensure that persons with pacemakers are not present in vicinity of the device during treatment.

The patient must not be left unattended during treatment.

Please see additional Important Safety Information on back page.

With Allergan, loyalty is rewarded

ALLERGAN PARTNER PRIVILEGES®



Best-in-class physician
loyalty program

CRYSTAL REWARDS® PROGRAM



Rewards participating
practices

BRILLIANT DISTINCTIONS®



Exclusive patient
loyalty program

Important Safety Information (continued)

Adverse effects may include, but are not limited to muscular pain, temporary muscle spasm, temporary joint or tendon pain, and local erythema or skin redness.

Consult the CoolTone™ User Manual for a complete list of Contraindications, Warnings, Precautions, and potential side effects. Treatment applications that deviate from the guidelines are not recommended.

Reference: 1. Data on file, Allergan.



COOLSCULPTING® the Snowflake Design, and COOLTONE™ are trademarks of ZELTIQ Aesthetics, Inc., an Allergan affiliate. Allergan® and its design are trademarks of Allergan, Inc. All other trademarks are the property of their respective owners. © 2019 Allergan. All rights reserved. coolsculptinghcp.com CTN126396 07/19 191811